




Figure 1A

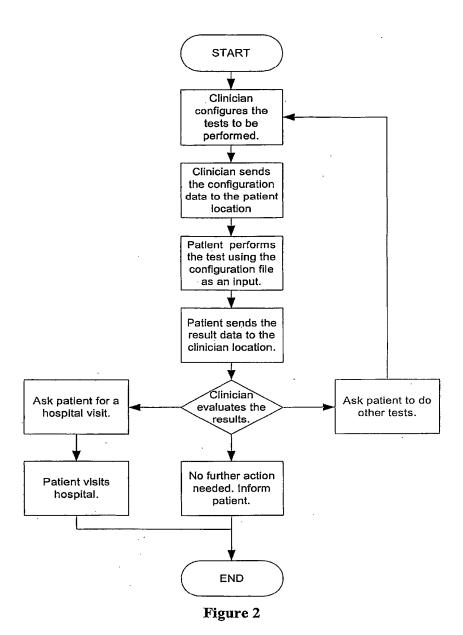

### Clinician application

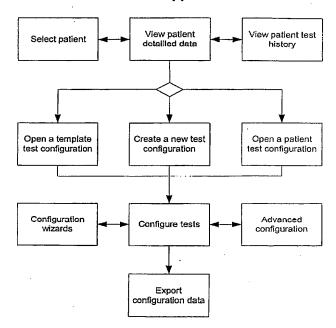

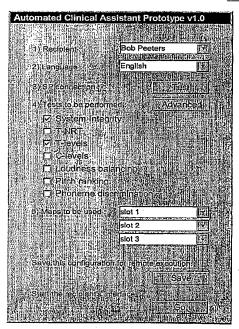

Automated Clinical Assistant Prototype v1.0

Test results for Bob Reelers

F. System Integrity. Dr.

F. System Integrity.

Figure 4

Figure 15


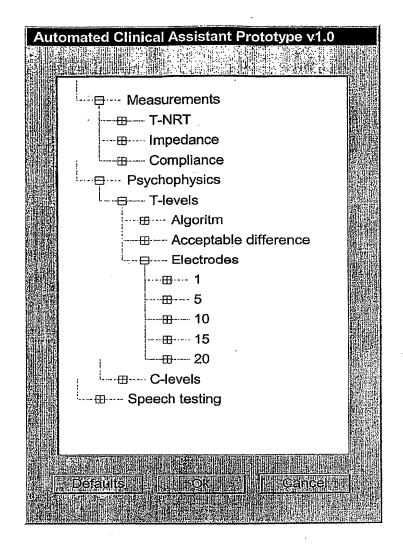


Figure 5

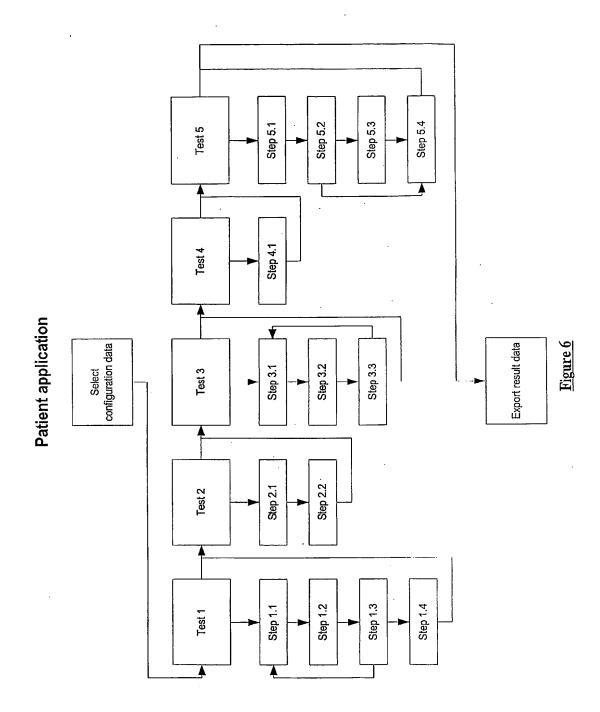

### NEXT

### Welcome, Bob Peeters.

We will lead you through different tests.

Ask the audiologist for help if something is unclear.

Press the NEXT button on the right bottom corner to continue.

## System integrity test.

The system will now check your system integrity.

Press GO to start the test.

Press any button or STOP when you hear something uncomfortable.

System integrity test in progress  Press any button or STOP when you hear something uncomfortable.  Progress indication	uncomfortable.
	STOP
Figure 9	

## System integrity test completed!

Press NEXT to continue.

## Psychophysics test.

The system will now stimulate soft tones.

Press NEXT to continue.

# Psychophysics test in progress...

Press PLAY to start the tone stimulation.

Press YES when you hear something.

Press NO when you hear nothing.

Press any button or STOP when you hear something uncomfortable.

You will be unable to hear some tones, since we also test at low levels.

STOP

2

YES

PLAY

Figure 13

## Psychophysics test completed!

Press NEXT to continue.

13/15

### All tests completed!

Congratulations, all tests are completed!

Tell your audiologist you have finished.

Press END to close the application.

